

CO-Oximeter
Calibration Verification Controls
(CVC 223)

Data Collection and Linearity Worksheets

Calibration Verification Controls (CVC 223)


for CO-Oximeters

Data Collection and Linearity Worksheet

Date: March 2, 19XX Operator: Mary Smith
 Instrument: Super X CO-Oximeter CVC 223 Lot #: 654321
 Instrument I.D.: 1A Expiration: 5/XX

tHb

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	<u>3.6</u>	<u>7.9</u>	<u>13.8</u>	<u>17.9</u>	<u>21.7</u>
Test 2	<u>3.8</u>	<u>8.0</u>	<u>14.2</u>	<u>18.0</u>	<u>21.9</u>
Test 3	<u>3.7</u>	<u>7.6</u>	<u>14.0</u>	<u>17.8</u>	<u>22.3</u>
Test Mean	<u>3.7</u>	<u>7.8</u>	<u>14.0</u>	<u>17.9</u>	<u>22.0</u>
Range	<u>3.4 - 4.6</u>	<u>7.3 - 8.9</u>	<u>13.1 - 14.9</u>	<u>16.9 - 18.9</u>	<u>20.9 - 23.1</u>
OK?	<input checked="" type="radio"/> Y or N	<input checked="" type="radio"/> Y or N	<input checked="" type="radio"/> Y or N	<input checked="" type="radio"/> Y or N	<input checked="" type="radio"/> Y or N

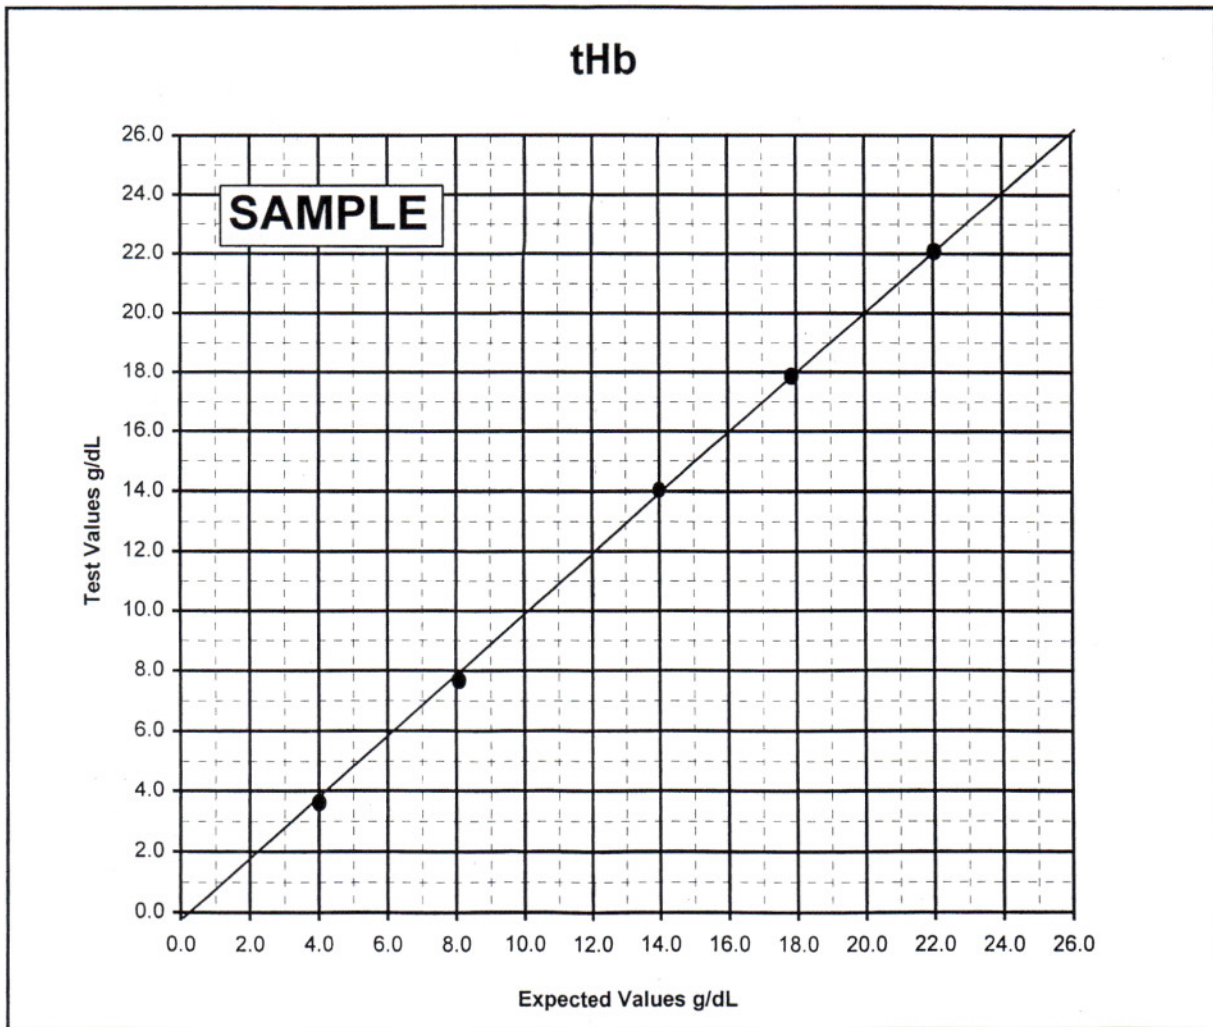

Comments: _____

Calibration Verification Controls (CVC 223)


for CO-Oximeters

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 223 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

tHb

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

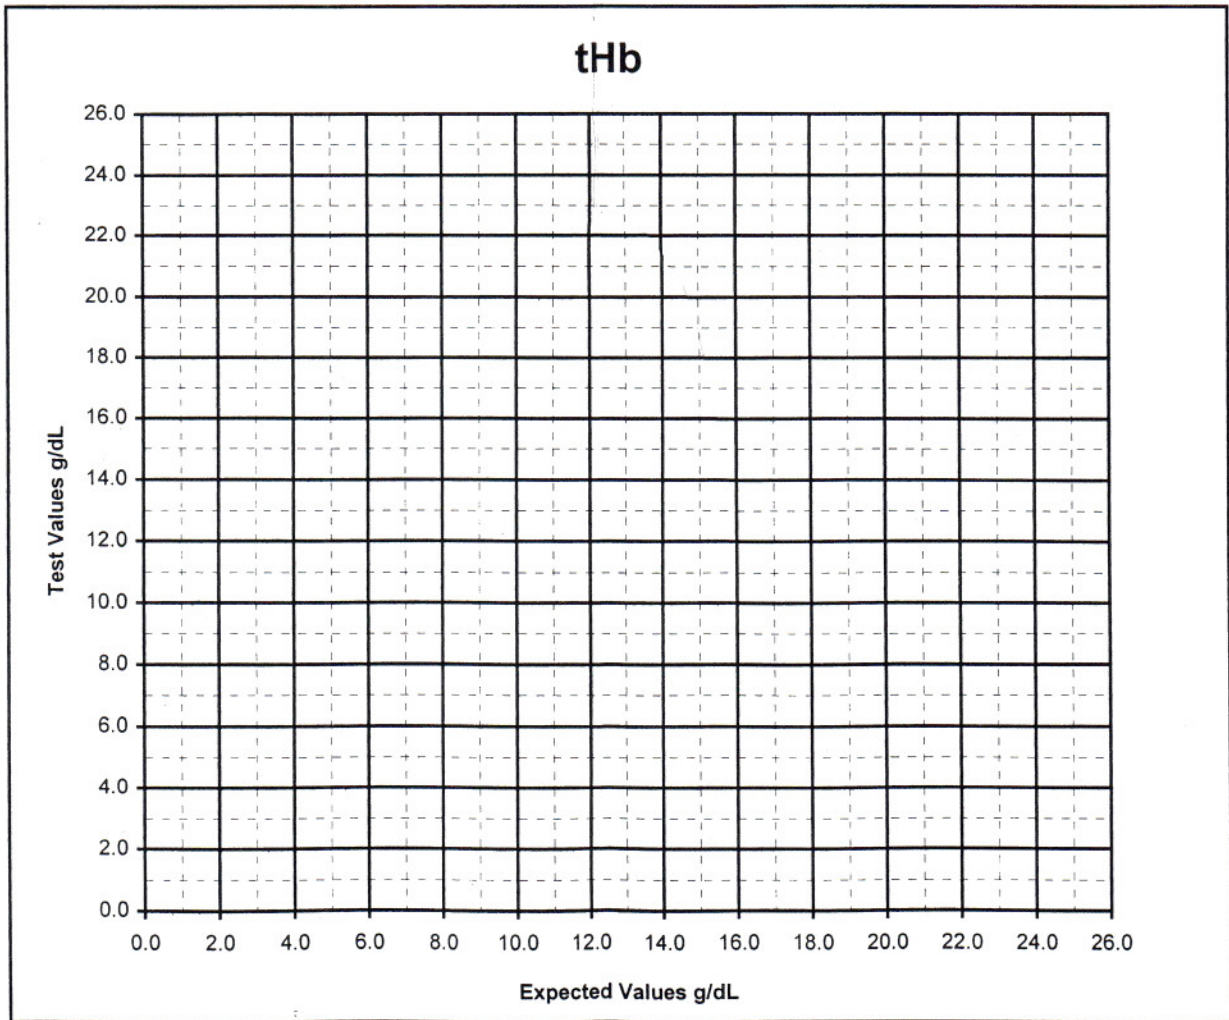

Comments: _____

Calibration Verification Controls (CVC 223)


for CO-Oximeters

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 223 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

O₂Hb

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

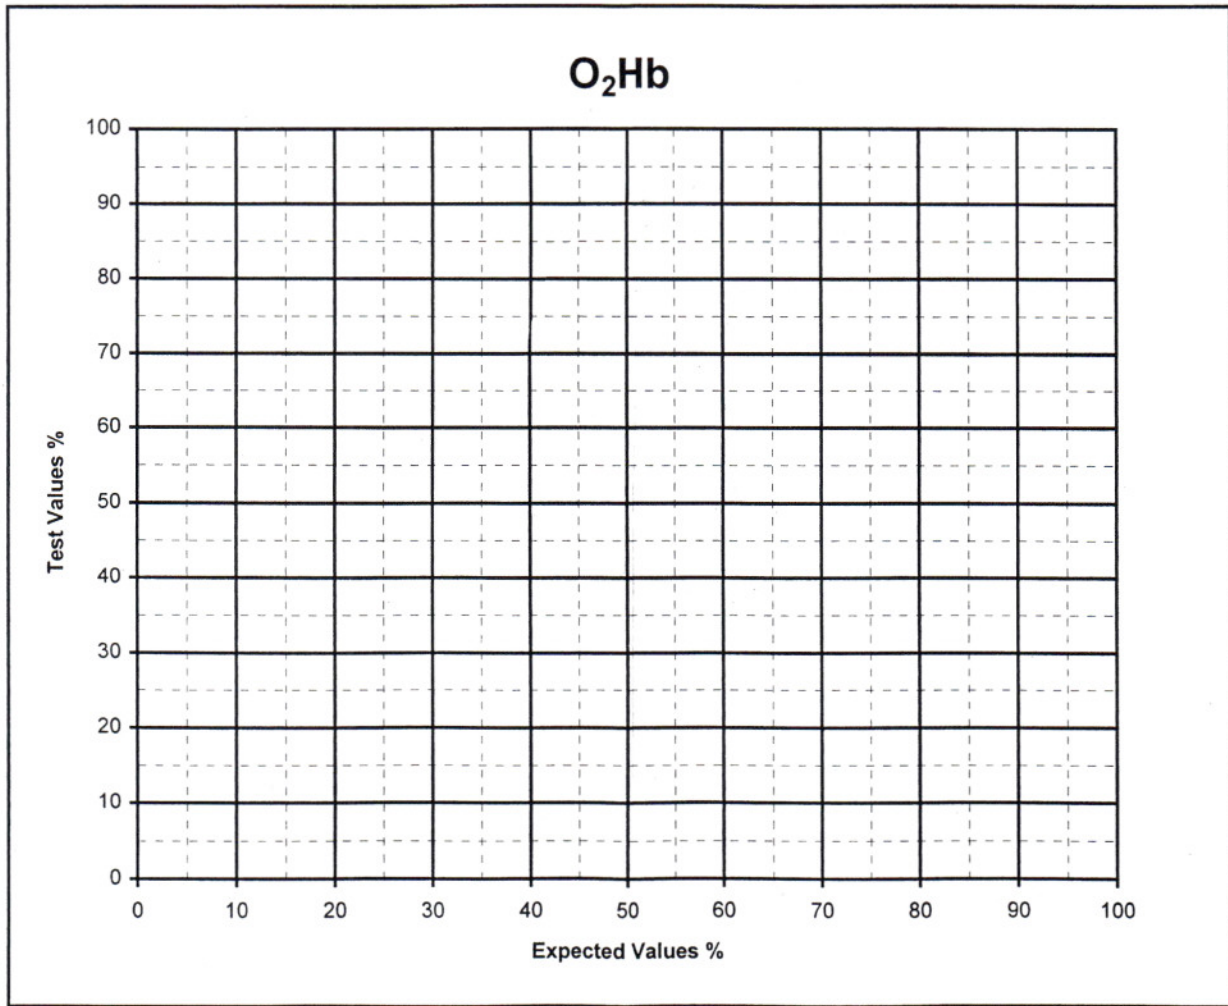

Comments: _____

Calibration Verification Controls (CVC 223)


for CO-Oximeters

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 223 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

COHb

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

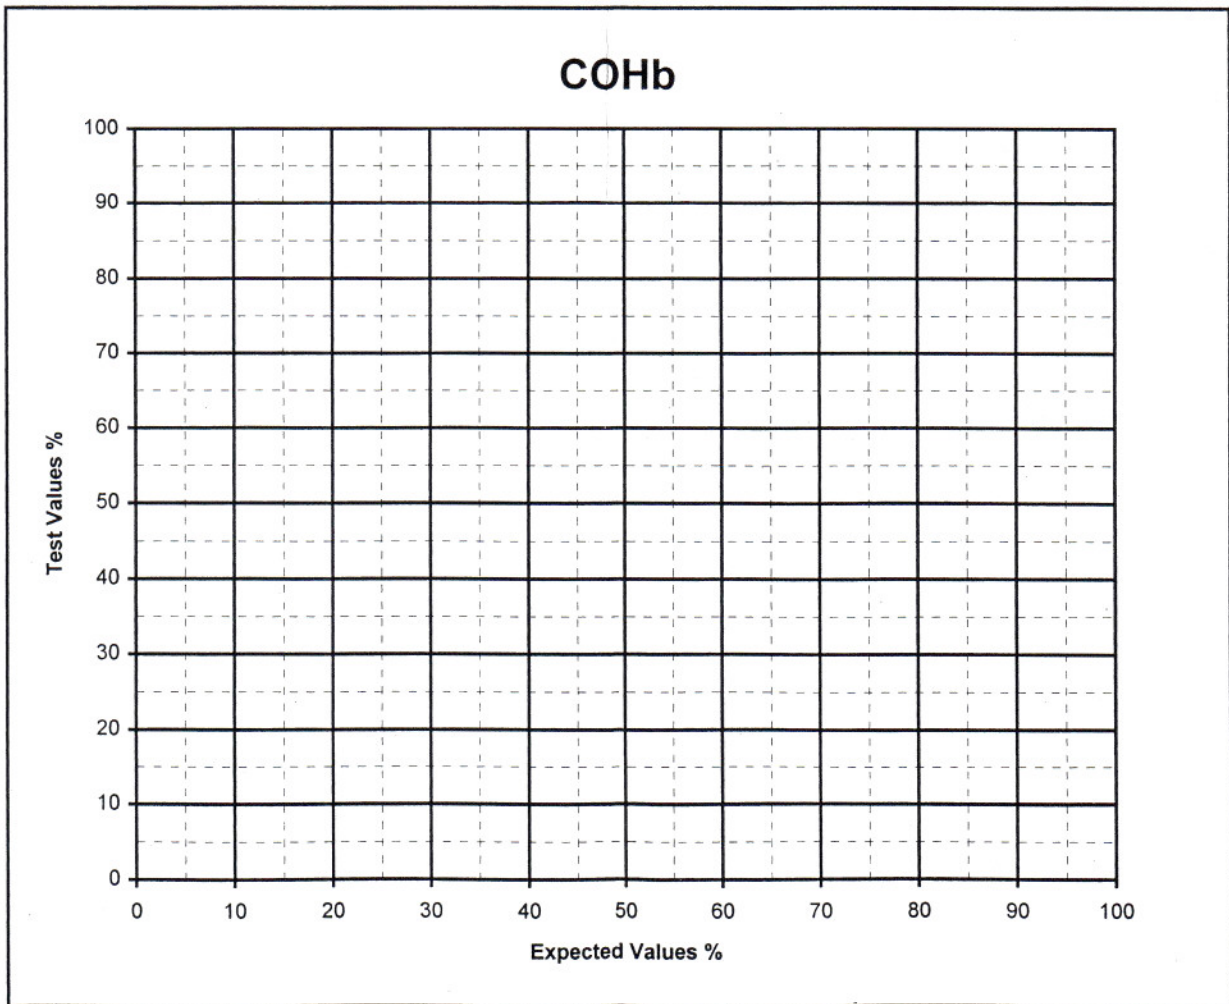

Comments: _____

Calibration Verification Controls (CVC 223)


for CO-Oximeters

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 223 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

MetHb

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

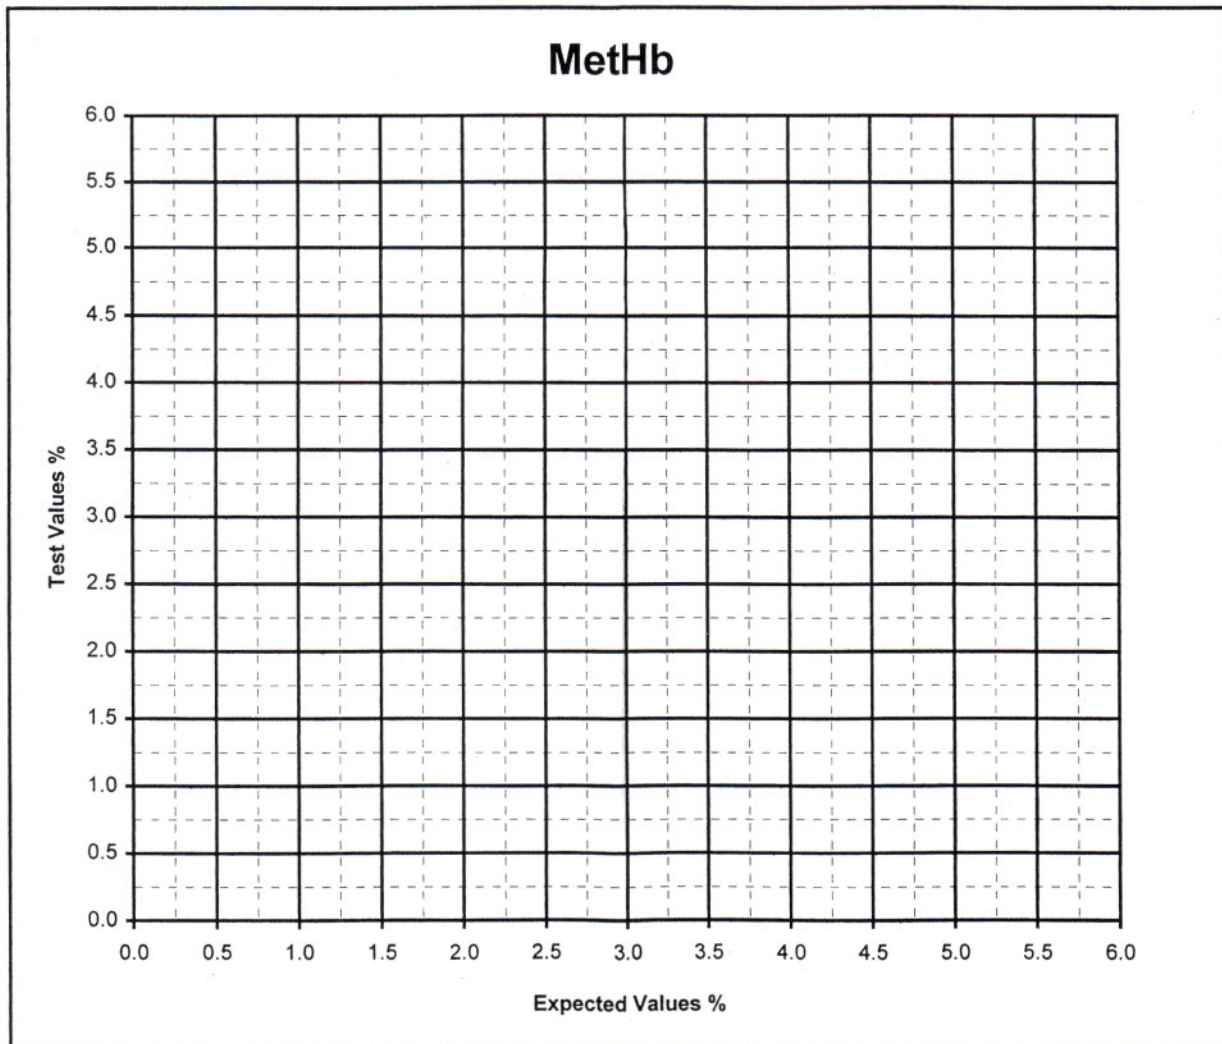

Comments: _____

Notes



7 Jackson Road, Devens, MA 01432-3900, 800-533-6162, Fax 978-772-9070