


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: March 2, 19XX Operator: Mary Smith
 Instrument: Super X Blood Gas Analyzer CVC 123 Lot #: 123456
 Instrument I.D.: 1A Expiration: 5/XX

	pCO₂				
	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	<u>92</u>	<u>70</u>	<u>43</u>	<u>21</u>	<u>10</u>
Test 2	<u>91</u>	<u>68</u>	<u>45</u>	<u>22</u>	<u>8</u>
Test 3	<u>96</u>	<u>68</u>	<u>42</u>	<u>19</u>	<u>8</u>
Test Mean	<u>93</u>	<u>69</u>	<u>43</u>	<u>21</u>	<u>9</u>
Range	<u>83 - 107</u>	<u>62 - 76</u>	<u>37 - 47</u>	<u>16 - 24</u>	<u>7 - 15</u>
OK?	<input type="radio"/> Y or N	<input type="radio"/> Y or N	<input type="radio"/> Y or N	<input type="radio"/> Y or N	<input type="radio"/> Y or N

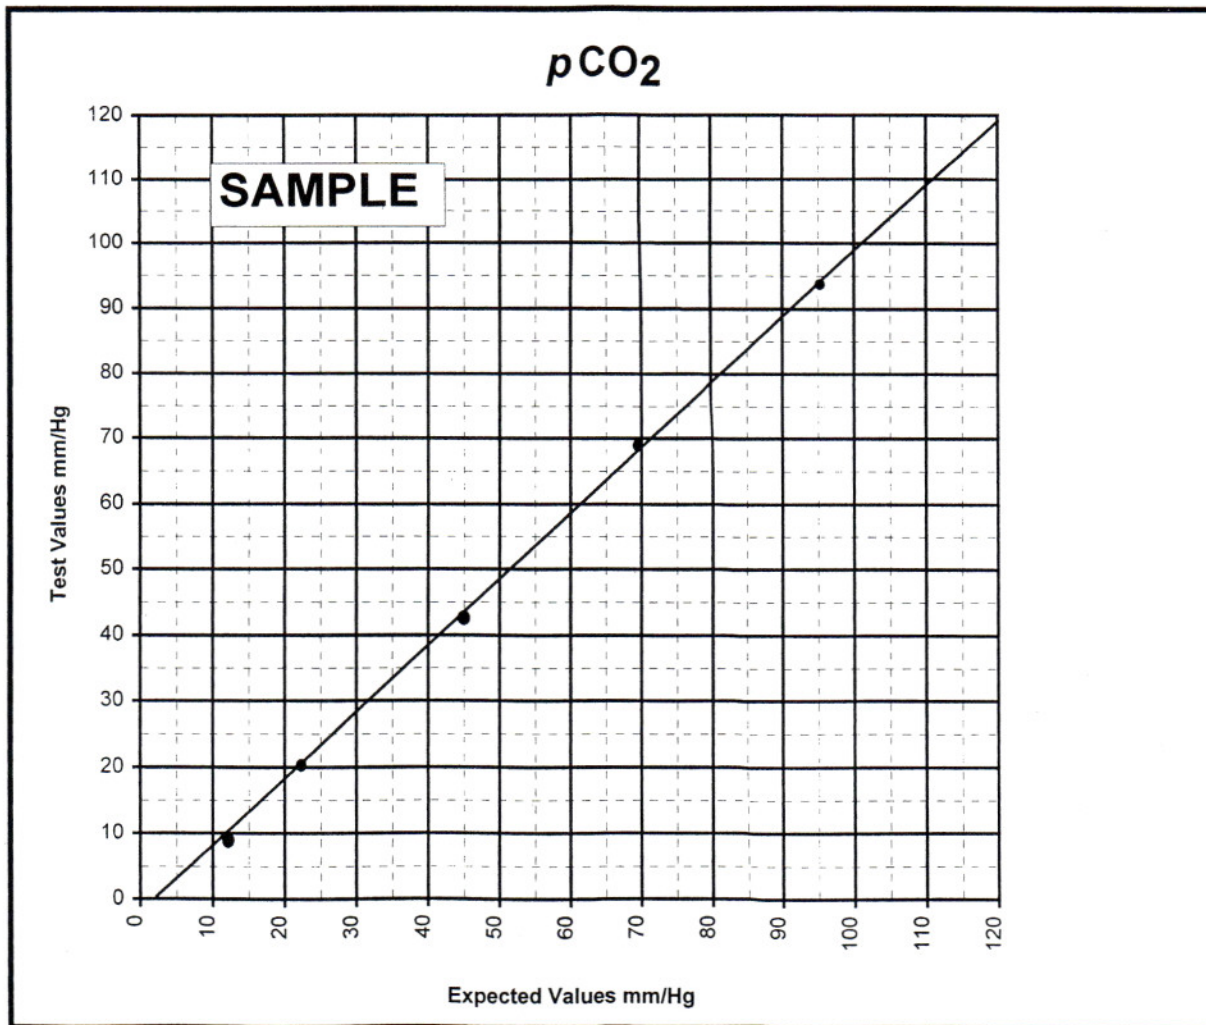


Comments: _____

Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

pH	Level	Level	Level	Level	Level
	1	2	3	4	5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

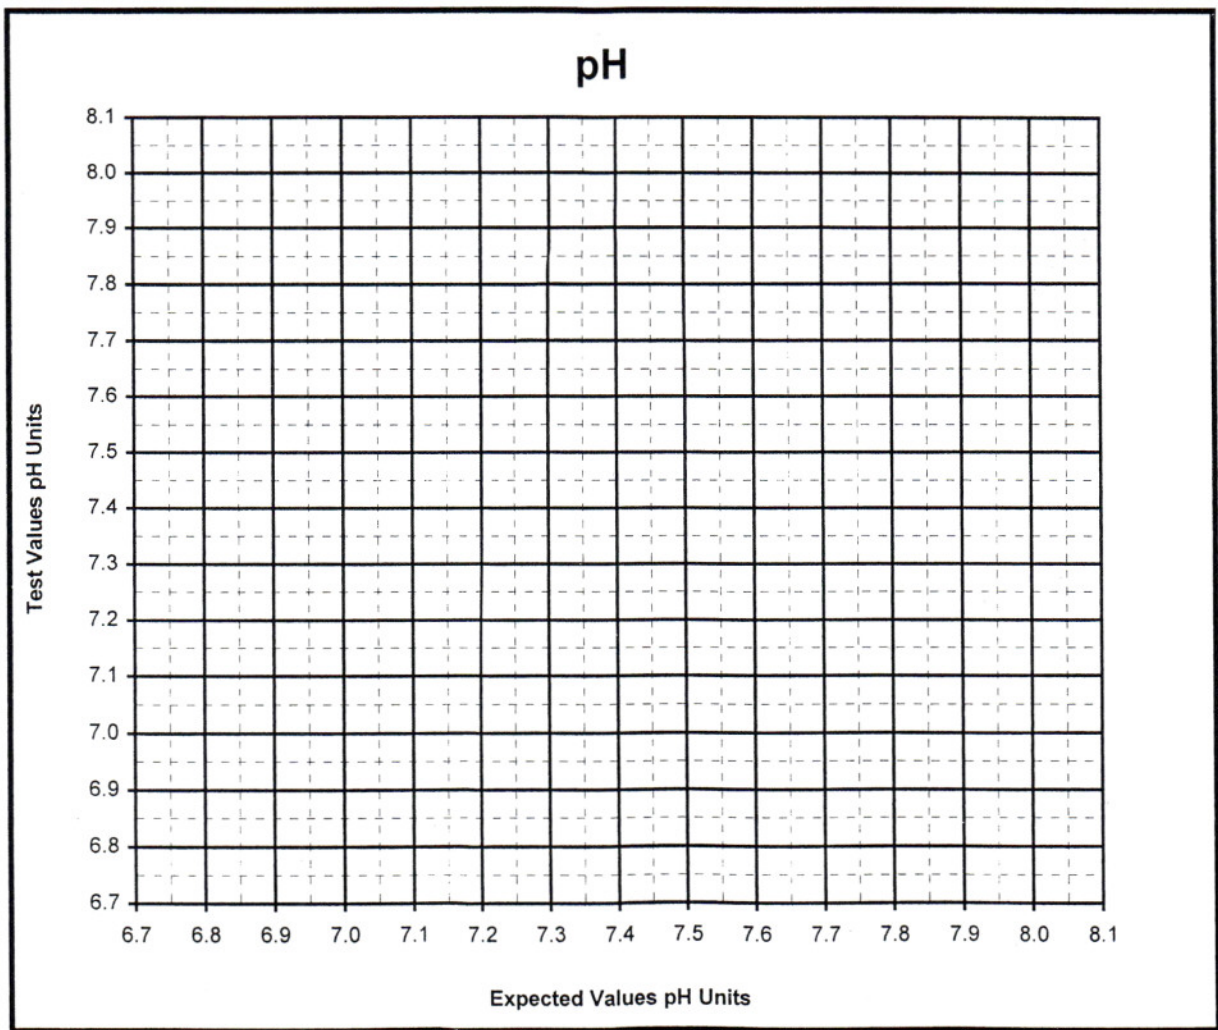

Comments: _____


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

pCO₂

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

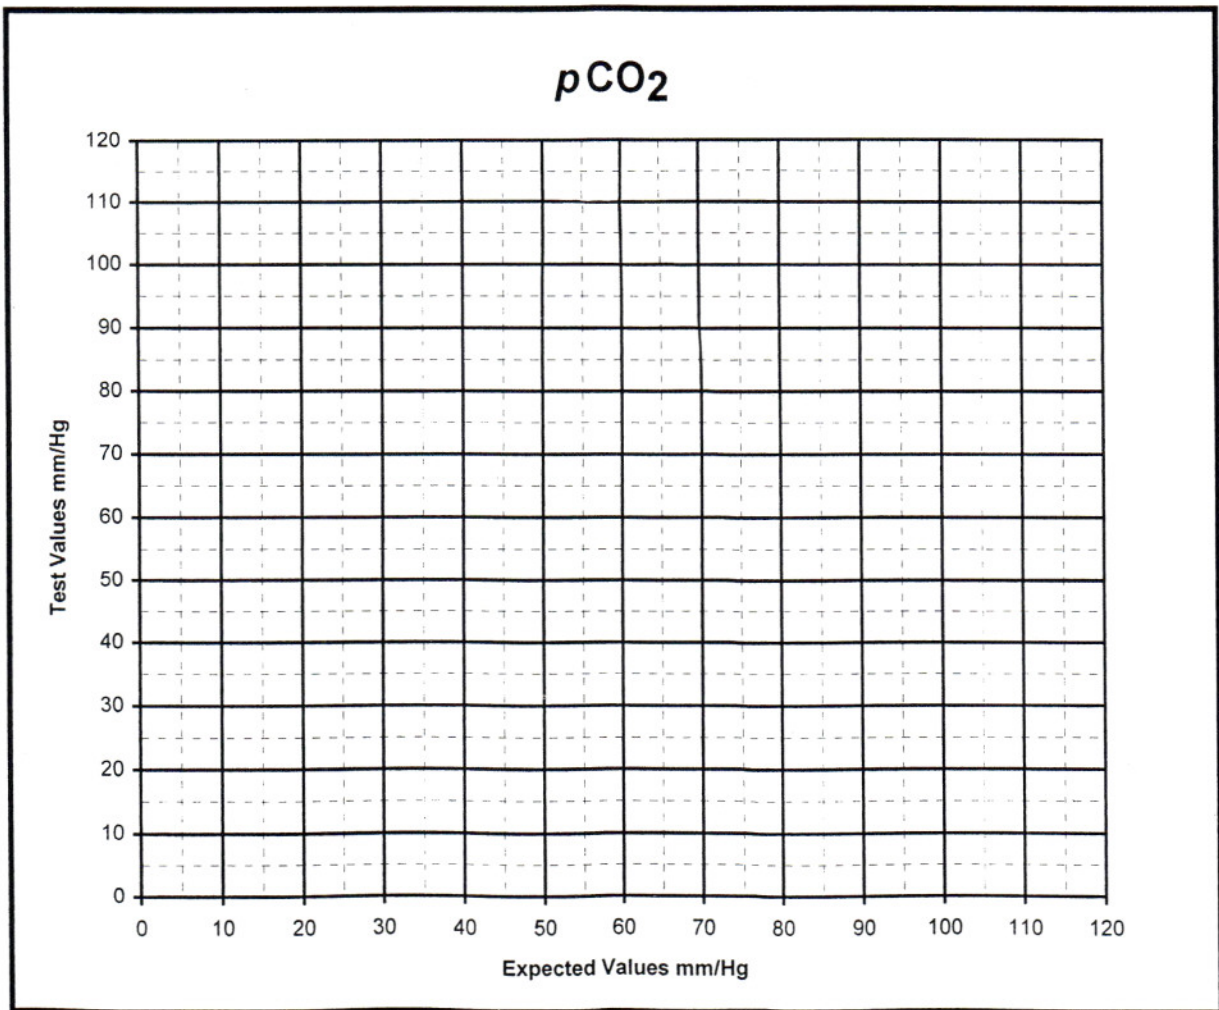

Comments: _____


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

pO₂

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

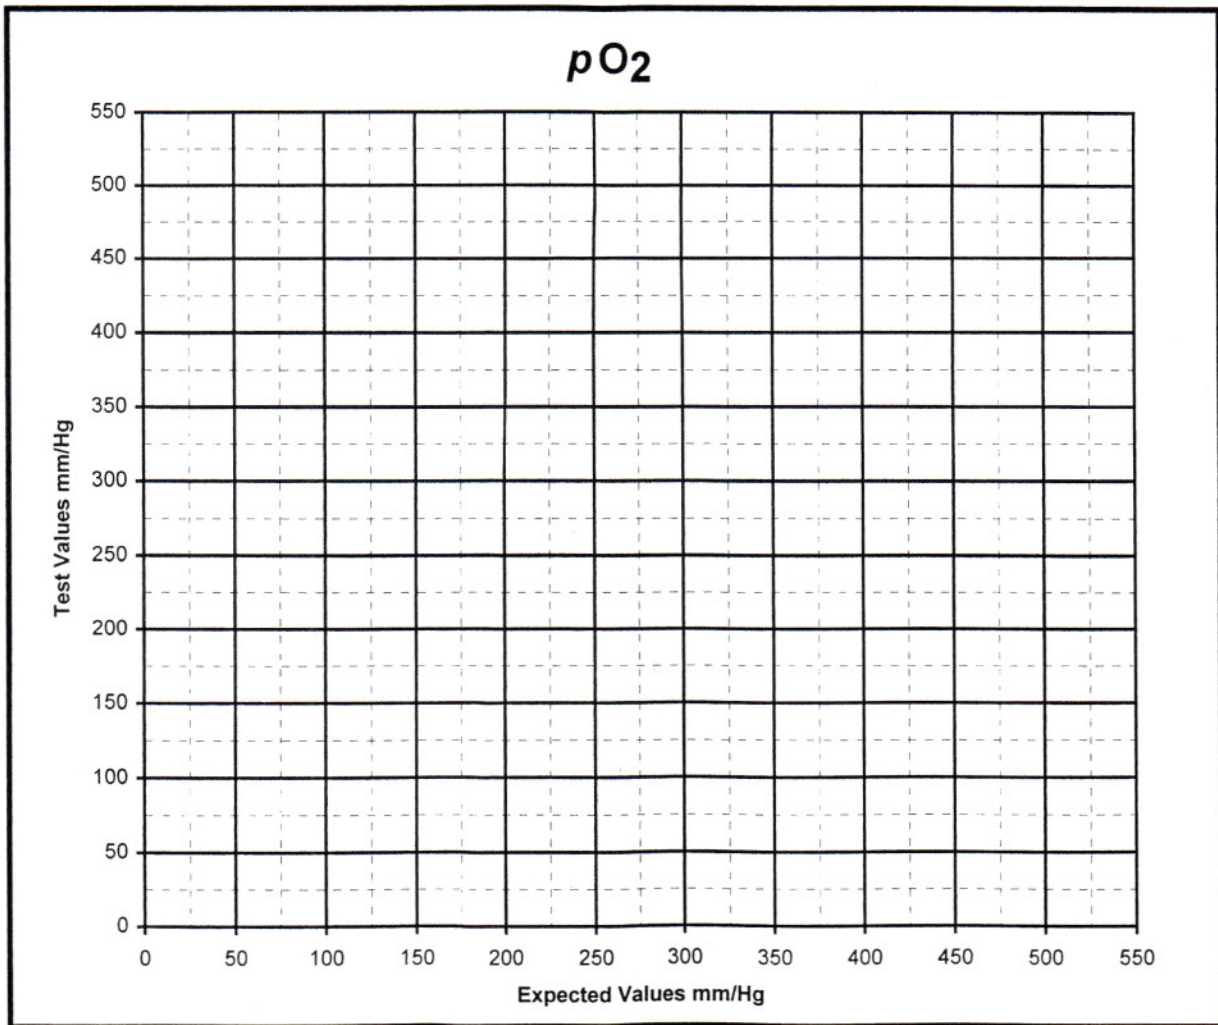

Comments: _____


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

Na⁺

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

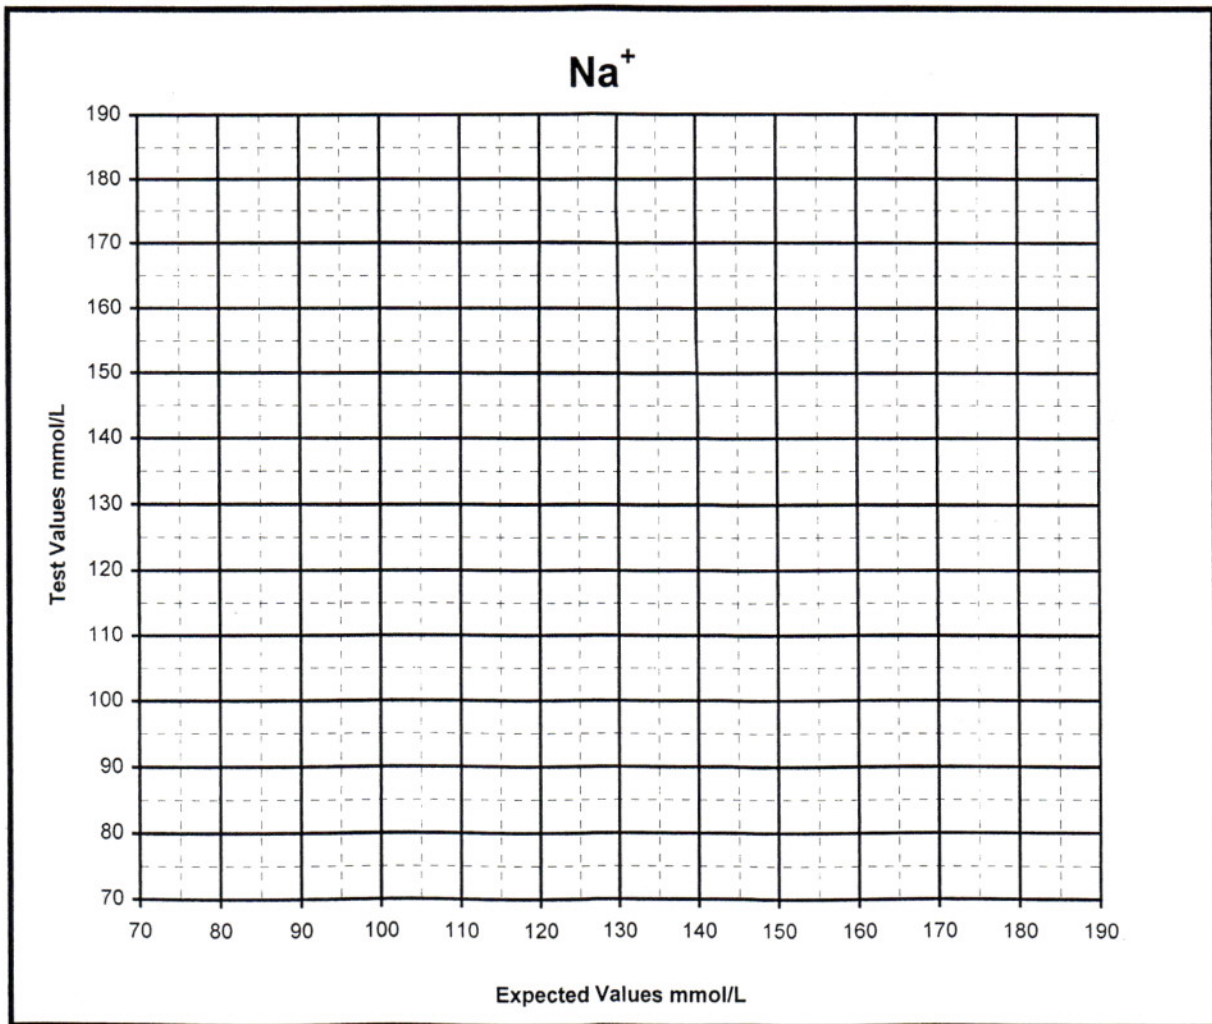


Comments: _____

Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

K⁺	Level	Level	Level	Level	Level
	1	2	3	4	5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

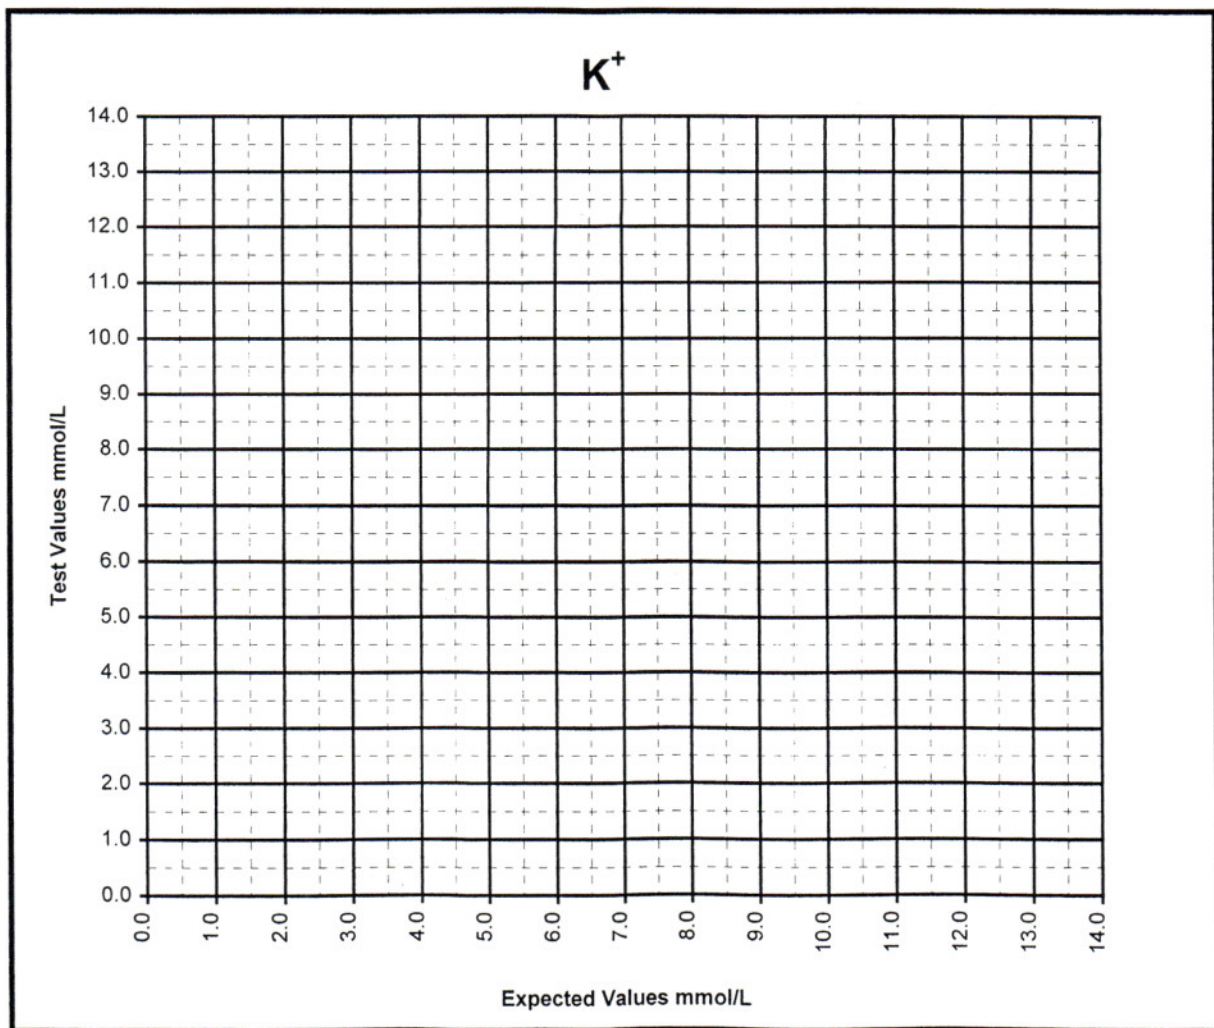

Comments: _____


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

Cl⁻

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

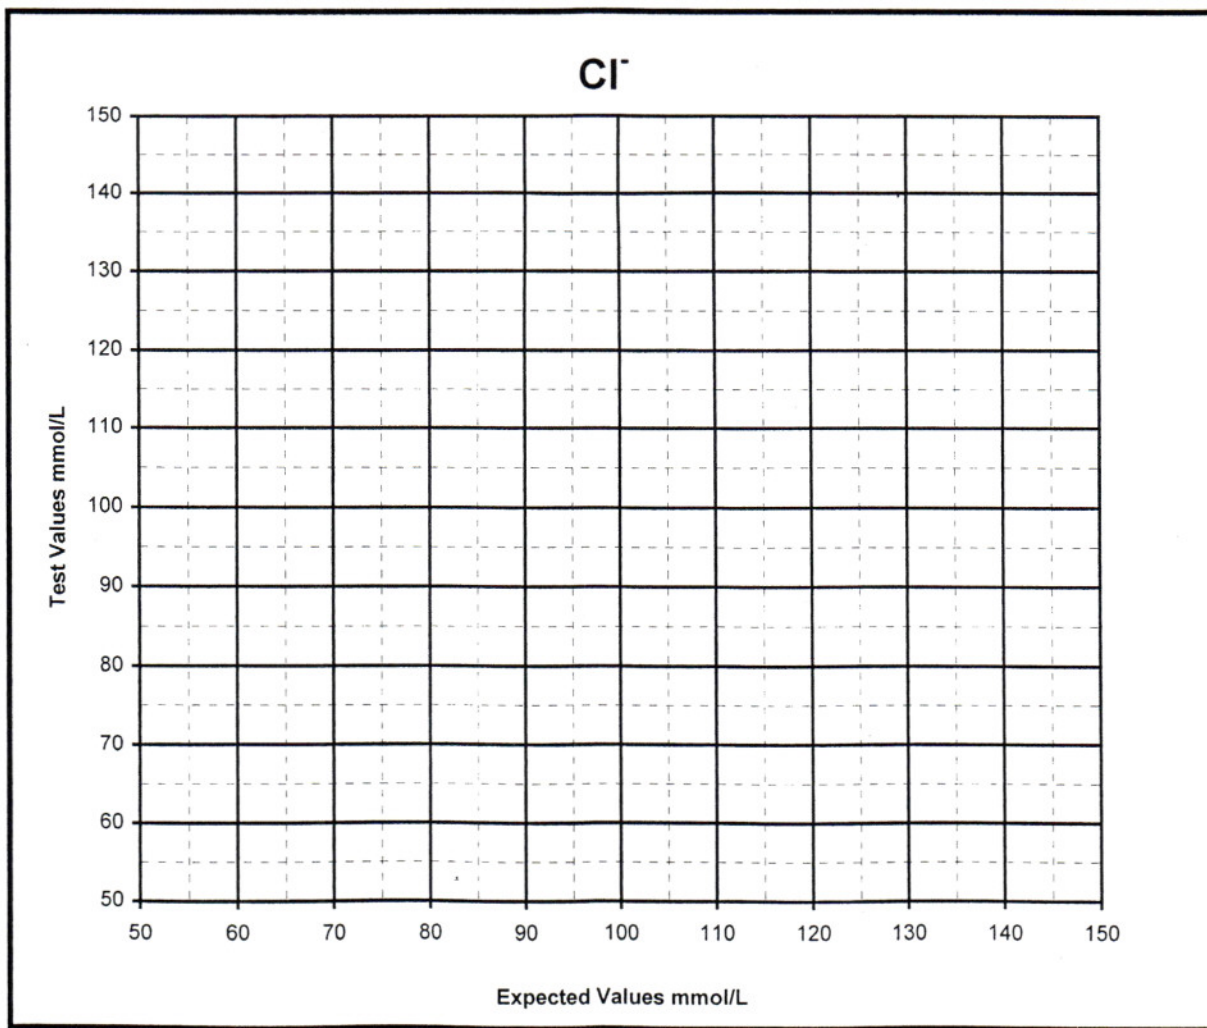

Comments: _____


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

Ca⁺⁺

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

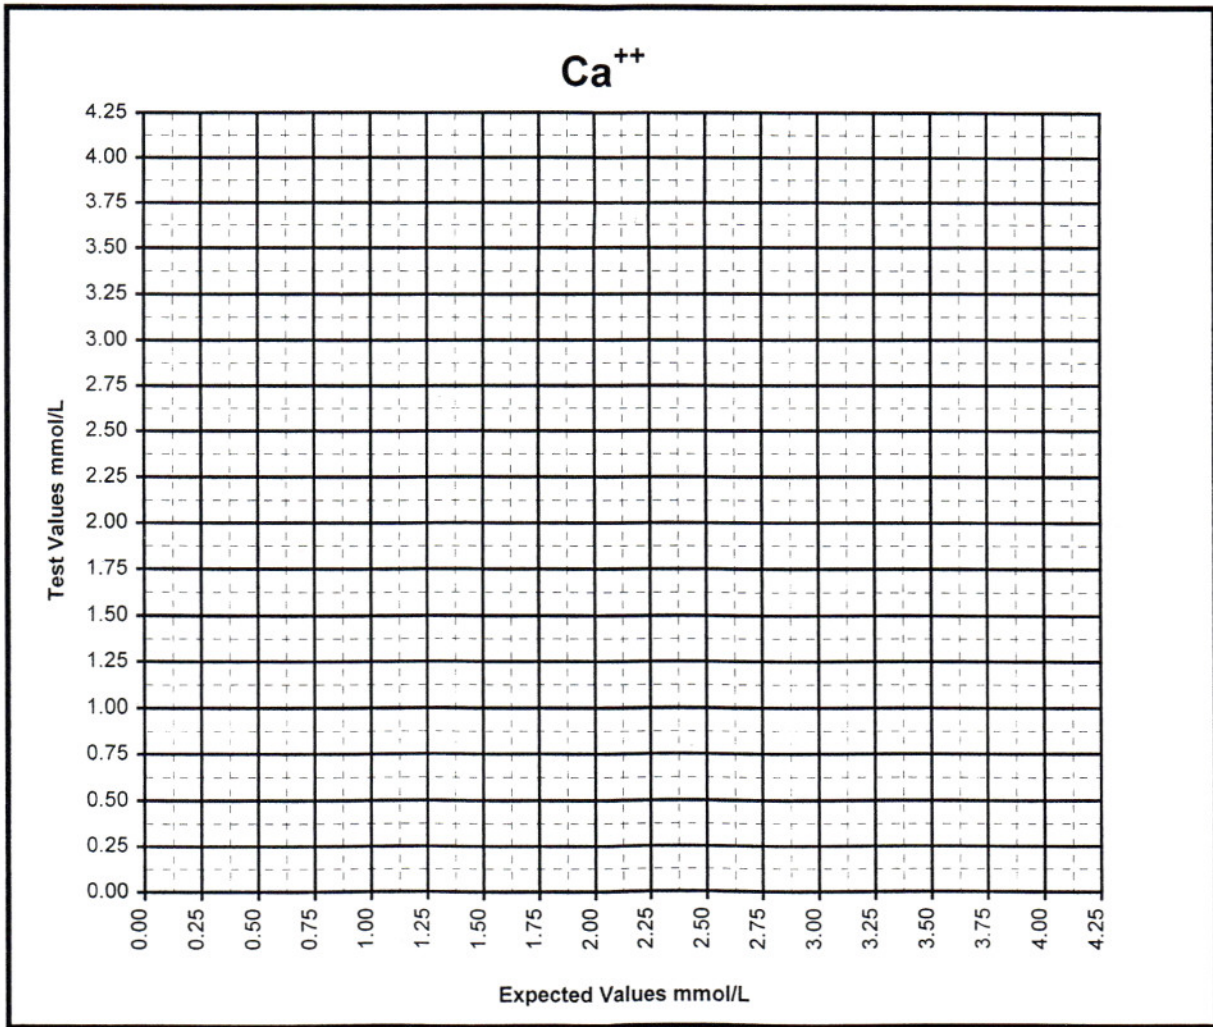

Comments: _____


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

Mg⁺⁺

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

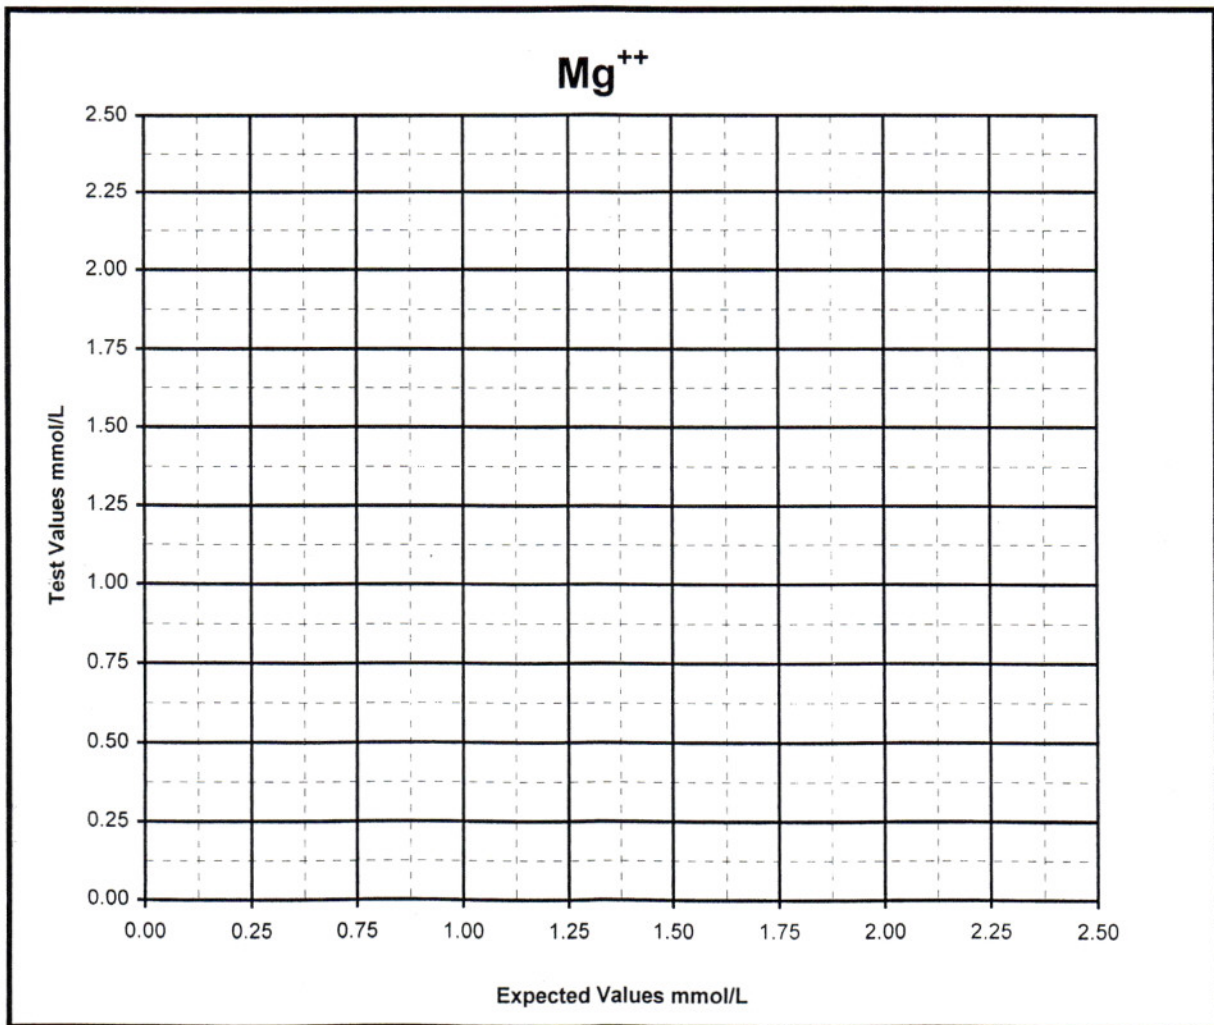

Comments: _____


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

Glu

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

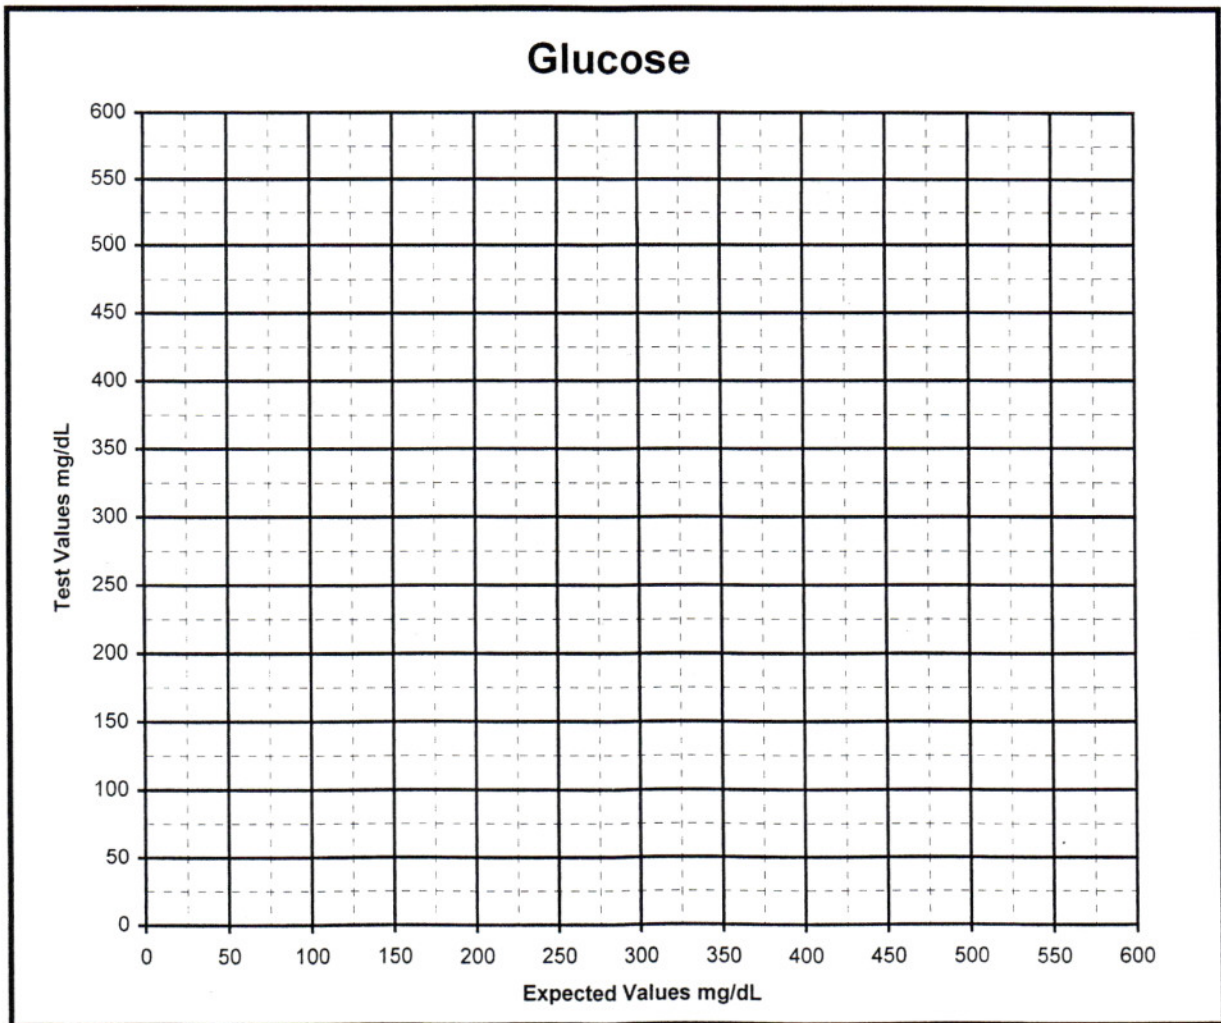

Comments: _____


Calibration Verification Controls(CVC 123)

Data Collection and Linearity Worksheet

Date: _____ Operator: _____
 Instrument: _____ CVC 123 Lot #: _____
 Instrument I.D.: _____ Expiration: _____

Lac

	Level 1	Level 2	Level 3	Level 4	Level 5
Test 1	_____	_____	_____	_____	_____
Test 2	_____	_____	_____	_____	_____
Test 3	_____	_____	_____	_____	_____
Test Mean	_____	_____	_____	_____	_____
Range	_____	_____	_____	_____	_____
OK?	Y or N	Y or N	Y or N	Y or N	Y or N

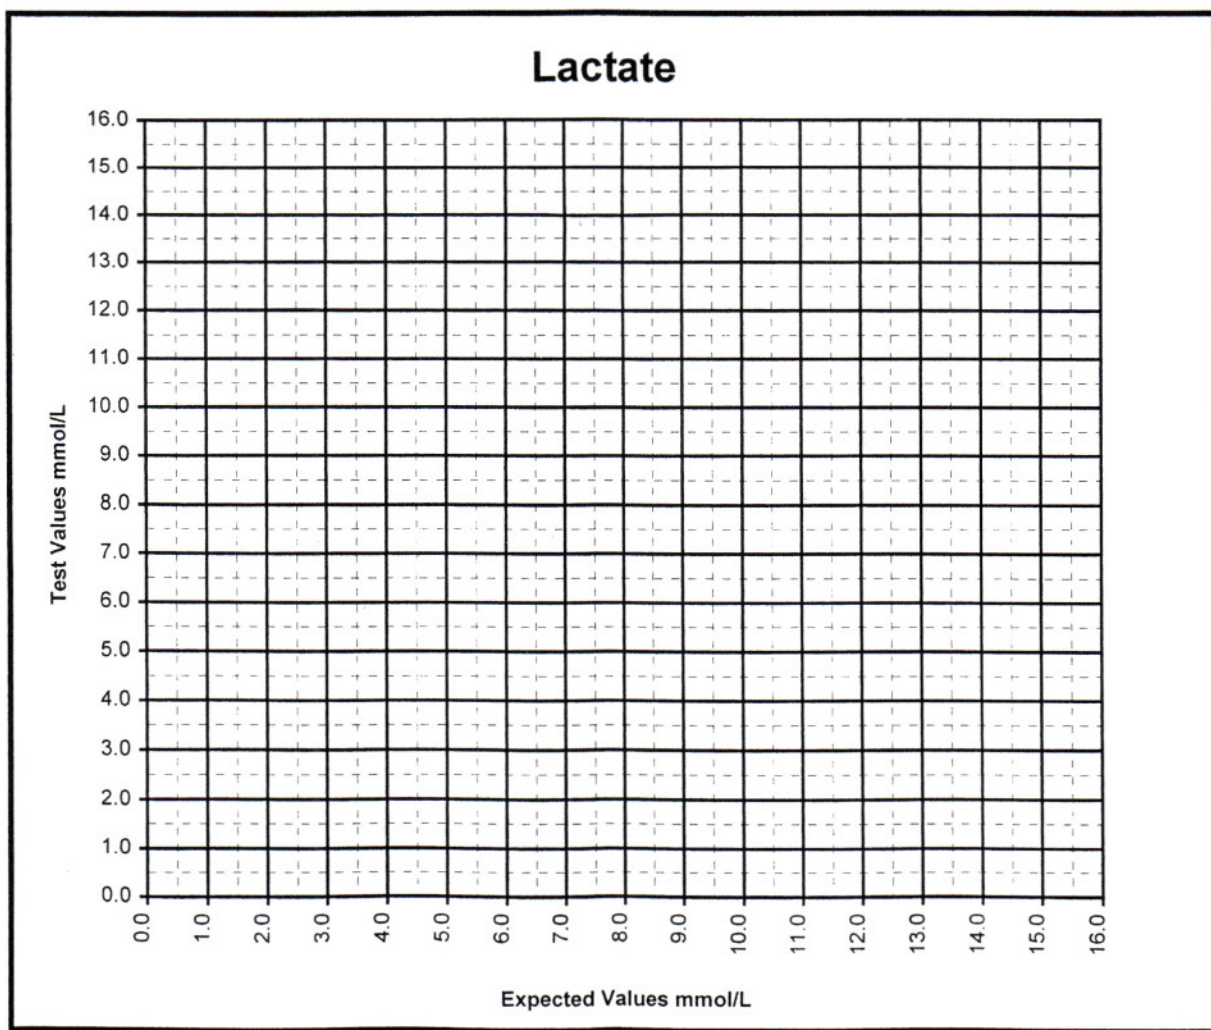

Comments: _____



7 Jackson Road, Devens, MA 01434, 800-533-6162, Fax 978-772-9071

Rev. A1021